

5301

OPERATING INSTRUCTIONS

Current Transducer

January 2012

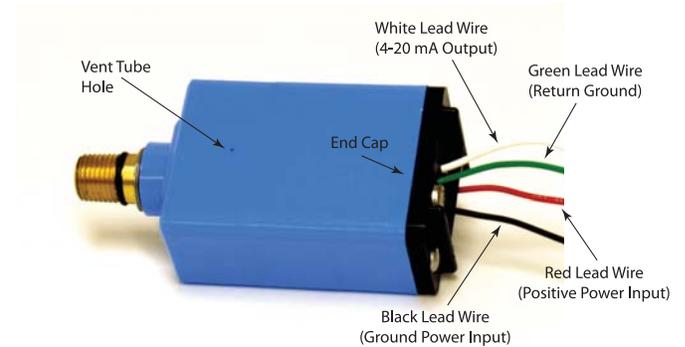
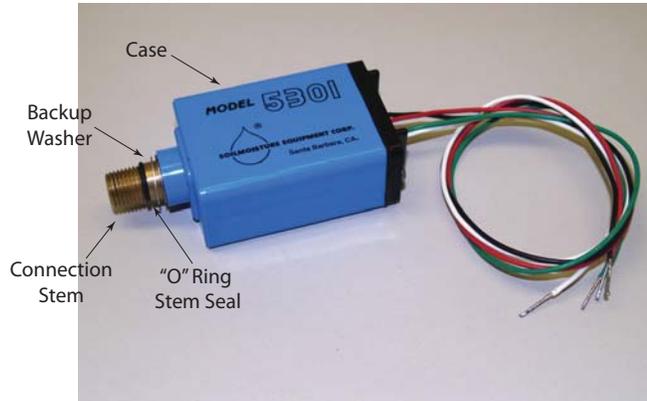


Fig. 1 - Current Transducer

UNPACKING	Page 2
SPECIFICATIONS	Page 2
ACQUAINT YOURSELF WITH THE PARTS	Page 3
MOUNTING THE TRANSDUCER SWITCH	Page 3
TESTING PRIOR TO INSTALLATION	Page 3
FIELD INSTALLATION	Page 4
SERVICING	Page 6
REPLACEMENT PARTS	Page 6

SOILMOISTURE EQUIPMENT CORP.

P.O. Box 30025, Santa Barbara, CA 93130 USA

Phone: 805-964-3525 - Fax: 805-683-2189 - Email: sales@soilmoisture.com

Website: <http://www.soilmoisture.com>

1





The Model 5301 Current Transducer is one of the most advanced, versatile, accurate means converting soil moisture tension measurements into a continuous analog output. The Current Transducer can be readily used with Model 2100 Model 2710, and Model 2725 Soilmoisture Tensiometers.

Special adapters are available to facilitate use of the Current Transducer with virtually any device which measures vacuum. The standard Current Transducer incorporates a 0-1 bar range transducer and solid state circuitry which allows continuous monitoring of soil moisture suction with time. Optional Transducer elements with operating ranges of 0 to 0.5 bars are also available. The special four-wire design assures excellent linearity, accuracy of output, and ease of installation.

UNPACKING

The Model 5301 Current Transducer shipped to you has been thoroughly tested before shipment. When packed, it was in perfect order. Unpack with care being sure to remove all packing material. Follow the instructions carefully in order to assure long, trouble-free service.

If Jet Fill Tensiometers were ordered at the same time, the Current Transducer may be mounted on the tensiometer, see Fig. 2 above. In this case, you will also receive separate instruction for the tensiometers. Handle the complete units with care and read all instruction information before installation.

NOTICE: ANY DAMAGE FOUND UPON RECEIPT SHOULD BE REPORTED IMMEDIATELY TO THE TRANSPORT CARRIER FOR CLAIM. IT IS IMPORTANT THAT YOU SAVE THE SHIPPING CONTAINER AND ALL EVIDENCE TO SUPPORT YOUR CLAIM.

Be sure to read all operating instructions thoroughly before operating unit.

SPECIFICATIONS

Power Requirement:	12 to 40 VDC at 50 mA (Internally regulated)
Operating Range:	0 to 1 bar (15 psi) vacuum
Operating Temperature Range:	32° to 140° F
Transducer Element:	Solid state differential silicon shear stress/strain gauge
Linearity:	.25% full scale max. (Typically +/- .1%)
Output:	4 to 20 mA
Hysteresis:	Less than 1%
Maximum Pressure Differential:	2 bars (30 psi)
Connecting Stem:	1/4" NPT Male
Accuracy:	+/- 1° of best fit curve

NOT LIABLE FOR IMPROPER USE

Soilmoisture Equipment Corp. is not responsible for any damage actual or inferred for misuse of improper handling of this equipment. The Current Transducer is designed to be used solely as directed, by a prudent individual under normal conditions in the applications intended for this instrument.


The 5301 Current Transducer involves proprietary electronic circuits and hardware. For repair of this instrument, the unit should be returned to Soilmoisture for any major repair work. Tampering with the Current Transducer in any unauthorized manner prior to return will void warranty and make the user liable for costs of repair.

Soilmoisture warrants all its products and related software to be free from defects for the period of one year.

the Vacuum Hand Pump can be inserted at the top of the unit. Connect the DC power source to the power leads of the Current Transducer and an ammeter to the output leads as described on page 1 under Acquaint Yourself With The Parts. When no vacuum is being applied, the ammeter should read 4 mA. In addition, the following calibration points are provided as check points:

Vacuum applied(cbs)	Ammeter Reading(mA)
0 cb	4 mA
25 cb	8 mA
50 cb	12 mA
75 cb	16 mA
100 cb	20 mA

The same relationship between Vacuum applied and Ammeter Readings is shown below graphically:

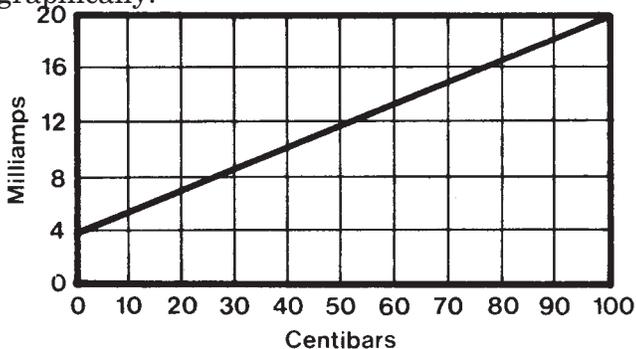


If the Model 2005G2 Vacuum Test Hand Pump is used in these tests, the vacuum level registered on the pump vacuum gauge will closely correlate with the ammeter readings shown above.

FIELD INSTALLATION


The tensiometer with attached Current Transducer is installed in the field in the same manner as vacuum gauge type tensiometers, and the specific instruction booklet covering the tensiometer used should be referred to for detailed information. Where the Current Transducer is monitoring important irrigation installations, precaution can be taken to protect the unit from physical damage as well as tampering. There are a variety of meter boxes that

are available on the open market that can be used. Fig. 5 shows a typical application. It is important to remember that tensiometer measurements are based on the moisture level surrounding the sensing tip of the tensiometer. For this reason it is essential that the tensiometer be located so that it is subject

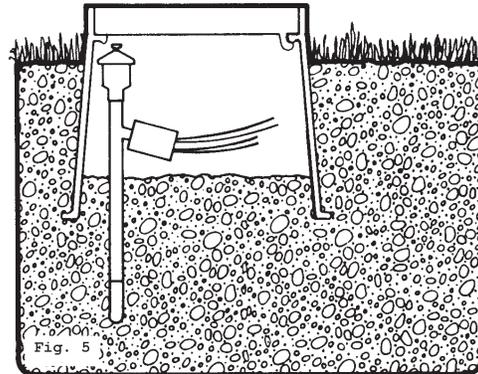

to the same amount of irrigation or rain water that is delivered to the total area under investigation.

In some installations it may be desirable to install the tensiometer at an angle, as shown in Fig. 6, to best expose the sensing tip of the tensiometer to conditions typical of the irrigated area.

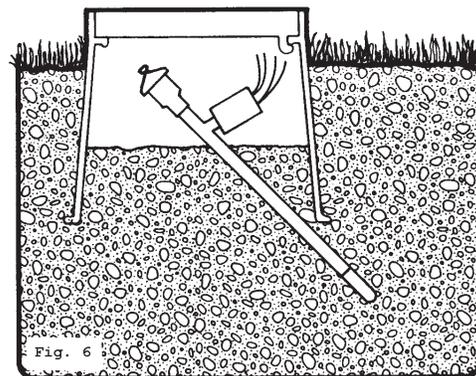

Electrical connection to the Current Transducer is made in the same general manner as to other electrical components of an irrigation system that are exposed to field conditions. Electrical connections must be water tight to avoid any electrical leakage during operation. The 12 to 40 VDC power supply is connected to the power (red and black) lead wires and an ammeter or data logger connected to the output (white and green) wires.

The current output from Model 5301 Current Transducer is preferred because the output signal is unaffected by random lengths of wire between the Current Transducer and data logging device for distances up to 1 mile.

Converting Current to Voltage

For applications in which a voltage output is preferred, the current output from Model 5301 can be converted to a voltage output using the well known equation $V = I * R$.

We know the current (I) varies from 4 mA (0.004 Amps) and 20 mA (0.020 Amps). If we want the 0.020 Amps to read 5 Volts, then we enter the values and compute the precision resistor value needed.

$R = 5.0 \text{ Volts} / 0.020 \text{ Amps} = 250 \text{ Ohms}$. For reference, we also calculate what voltage value we will get for the 0.004 Amps ($V = 0.004 \text{ Amps} * 250 \text{ Ohms} = 1 \text{ Volt}$). Our 4-20 mA will be converted to 1-5 Volts when we use a 250 Ohm precision resistor.

Another example might be we want 10 Volts output. Now $R = 10.0 \text{ Volts} / 0.020 \text{ Amps} = 500 \text{ Ohms}$ and 0.004 Amps will yield $V = 0.004 \text{ Amps} * 500 \text{ Ohms} = 2 \text{ Volts}$. Our 4-20 mA will be converted to 2-10 Volts using a precision 500 Ohm resistor.

Calibration Capacity

Note that Model 5301 now comes with calibration capability. Units are calibrated at the factory, but if it is found that additional calibration or adjustment is needed, it is now possible for you to do.

There are 2 calibration screws on the back side of the Transducer: the screw closest to the BLACK wire is the "Offset"; the screw closest to the RED wire is the "Gain".

Offset is set to 4.00 and a small amount of drift from 3.8 to 4.2 is normal. With no vacuum on the transducer, turn the screw clockwise to increase the value and counter-clockwise to decrease the value.

To adjust gain, it is necessary to subject the transducer to a vacuum. If the transducer is the B.5 Model, then pull 50 cb of vacuum and adjust the gain to 12. Again, a small amount of drift in between

11.8 and 12.2 is normal.

Other values besides 50 cb could also be used and need to be calculated depending on the Transducer and the values selected:

- No vacuum is equal to 4.00 mA
- Full vacuum (B1) is 20 mA
- Half vacuum (B.5) is 20 mA
- In between values are linear.

SERVICING

The only servicing required is for occasional air removal from the tensiometer to maintain a high sensitivity. Specific instructions on the tensiometer should be referred to for this purpose. The Current Transducer is of advanced electronic design and no repairs should be attempted in the field. The Current Transducer must be returned to the factory or authorized factory dealer for repairs. Opening the transducer housing and breaking the hermetic seal will void our guarantee.

REPLACEMENT PARTS

- M801X013 "O" Ring Seal (Connecting Stem and Set Point Covers)
- RW090CAS Backup Washer