

OPERATING INSTRUCTIONS

08.13 WET SIEVING APPARATUS



Contents

On these operating instructions	2
1. Introduction.....	2
2. Applications.....	2
3. Operating principles.....	2
4. Procedure	3

On these operating instructions



When the symbol shown on the left is placed before a piece of text, this means that an important instruction follows.



When the symbol shown on the left is placed before a piece of text, this means that an important warning follows pointing out a risk of injury to the user or damage to the device. The user is always responsible for its own personal protection.

Text

Text in italics means that the actual text is shown on the display screen or instrument.

1. Introduction

The wet sieving apparatus is used to determine the aggregate stability of a soil, which is the resistance of soil structure against mechanical or physico-chemical destructive forces.

Soil structure is one of the main factors controlling plant growth by its influence on root penetration, soil temperature and gas diffusion, water transport and seedling emergence and therefore it is an important soil characteristic for farmers.

Soil structure is defined by the combination or arrangement of primary soil particles into compound elements, which are separated from adjoining structural elements by surfaces of weakness.

Soil texture, soil structure, and the type of clay mineral, organic matter content and type, cementing agents and cropping history influence the aggregate stability. Among the mechanical destructive forces are soil tillage, impact of heavy machinery, treading by animals and raindrop splash. Physico-chemical forces are e.g. slaking, swelling and shrinkage, dispersion and flocculation.

Slaking is the process of structure breakdown under the influence of wetting of soil aggregates, due to swelling of clay minerals, dissolving of cementing agents, air explosion or reduction in pore water suction. Slaking may result in the formation of a superficial crust, reducing water infiltration and enhancing sediment loss by downward transportation with surface runoff water.

2. Applications

Due to the impact of aggregate stability on plant growth and soil loss, applications of the wet sieving apparatus are the fields of agriculture and land conservation. This method to determine aggregate stability will be especially useful for researchers and scientists on soil erosion, land degradation and conservation, agriculture, sustainable agriculture.

Scientists on salinization problems may have advantage determining wet aggregate stability using wet sieving, to control deterioration of soil structure or to determine possible impacts of amelioration practices on aggregate stability.

Determining aggregate stability will give information on the sensitivity of soils to water and wind erosion, which might be prevented e.g. by mulching the soil surface. Information on soil aggregate stability will improve tillage programs, adapted to the specific soil type and crop demands.

3. Operating principles

The wet aggregate stability is determined on the principle that unstable aggregates will break down more easily than stable aggregates when immersed into water.

To determine the stability, 8 sieves (with 60 Mesh screen) are filled with a certain amount of soil aggregates. These sieves are placed in a can filled with water, which will move up and downward for a fixed time. Unstable aggre-

gates will fall apart and pass through the sieve and are collected in the water-filled can underneath the sieve. After this fixed time, the cans are removed and replaced by new water filled cans. Now, all aggregates are destroyed. Sand grains and plant roots will remain on the sieve and only aggregates are considered. After drying the cans with the aggregates, the weight of both stable and unstable aggregates can be determined.


Dividing the weight of stable aggregates over total aggregate weight gives an index for the aggregate stability.

To prevent slaking of the aggregates when putting the filled sieves into the water filled cans, the aggregates are pre-moistened with water vapour, using a humidifier or a very fine plant sprayer.


4. Procedure

Determining aggregate stability using the wet sieving apparatus:

1. Weigh 4.0 grams of 1- to 2- mm air-dried aggregates into the sieves.
2. Pre-moistened the aggregates. Depending on the sample leave the sample 5-10 minutes before submerging them.
3. Place the sieves in the sieve holder.
4. Place the weighed (numbered) cans.
5. Place the sieve holder on de build-in stop.

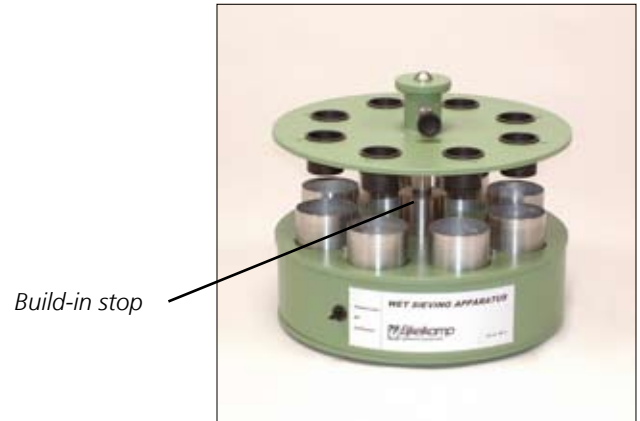

6. Place sufficient distilled water into the cans to cover the soil. The water can be put into the cans through the special can-fill openings in the sieve holder. During the sieving it is important that the samples are moved under water (so add enough water to the boxes).

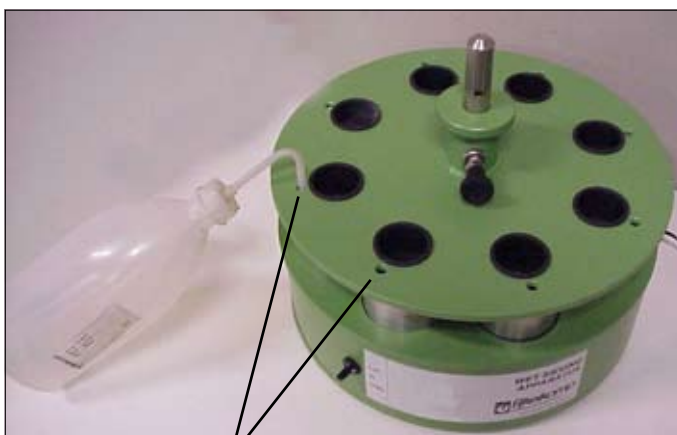


Can-fill openings




- Place the sieve holder in the working position by putting the sieve holder in the second hole on the shaft

Second hole on the shaft

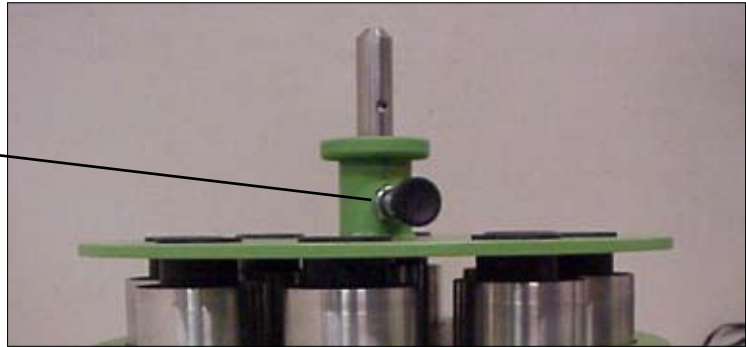

- Check if the mains switch is in the "Off" position
- Put the Adapter into a wall plug
- Start the motor by putting the mains switch into "3 min" position and allow it to raise and lower the sieve-holder for 3 min. \pm 5 s. (stroke = 1.3 cm, at about 34 times/min)
At the end of this time the motor will stop automatically.
- Raise the sieve holder out of the water and place it in the leak out position, by putting the sieve holder in the sieve holder in the first hole on the shaft.

First hole on the shaft

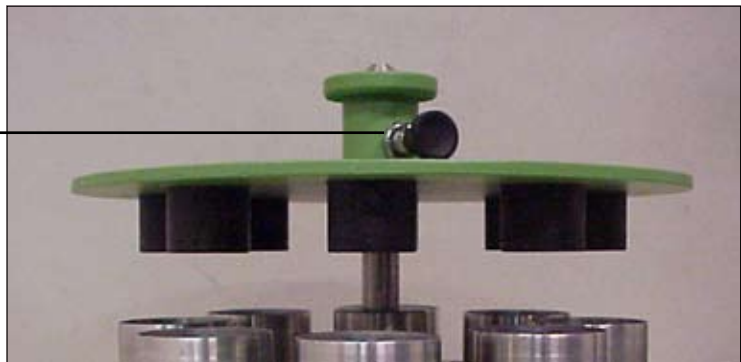

When there is no water leaking out of the sieves anymore, than take the (numbered) cans (containing the particles and aggregate fragments that have broken loose from the aggregates and come through the sieves) on a tray.

- Replace these cans with another set of weighed (numbered) cans
- Fill the cans with a dispersing solution (containing 2 g sodium hexametaphosphate/L) for soils with pH > 7 or 2 g NaOH/L for soils with pH < 7. (for the filling procedure see point 4 and 5).
- Place the sieve holder in the working position
- Start the motor by putting the mains switch into "Continue" position and continue sieving until only sand particles (*and root fragments*) are left on the sieve. If some aggregates remain stable after 5 to 8 min of sieving in the dispersing solution, stop the sieve by putting the mains switch in the "Off" position, and rub them across the screen with a rubber tipped rod until they are disintegrated.
- Continue sieving until materials smaller than the screen openings have gone through.



To disperse the aggregates can take some time (the more clay the longer it takes); there is no standard reacting time. Use of the reagent in combination with washing is the best method to be sure that all the aggregates are dispersed.

- Raise the sieve holder and place it in the leak out position.
When there is no dispersion solution leaking out of the sieves anymore, than take the (numbered) cans and

place them on a separate tray.

These cans contain the materials from the aggregates that were stable, except for sand particles too large to get through the screen.

18. Both sets of cans are placed in a convection oven at 110 °C until the water has evaporated.
19. The weight of the materials in each can is then determined by weighing the can, plus contents, and subtracting the weight of the can. In the cans, which were filled with dispersing solution, there will be 0.2 g of the dispersing solute along with the soil. Consequently, 0.2 g should be subtracted from the weight of the contents to obtain the soil weight.
20. The fraction stable is equal to the weight of soil obtained in the dispersing solution cans divided by the sum of the weights obtained in the dispersing solution cans and distilled water cans.

Dispersion of the aggregates may also be achieved using an ultrasonic probe, in which case, the dispersing solution can be distilled water rather than the sodium salt solution, which eliminates the need for the 0,2 g correction indicated in step 19.

The test procedure is now:

Step 1 to 10 see above

11. Fill the cans with distilled water (for the filling procedure see point 4 and 5)
12. Then held the ultra sonic probe into the water for 30 s at a medium frequency
13. Place the sieve holder in the working position
14. Start the motor by putting the mains switch into "*Continue*" position and continue sieving until only sand particles (and root fragments) are left on the sieve. If some aggregates remain stable after 5 to 8 minutes of sieving in the dispersing solution, stop the sieve by putting the mains switch in the "*Off*" position, and rub them across the screen with a rubber tipped rod until they are disintegrated.
15. Continue sieving until materials smaller than the screen openings have gone through.
16. Raise the sieve holder and place it in the leak out position.
When there is water leaking out of the sieves anymore, than take the (numbered) cans and place them on a separate tray.
These cans contain the materials from the aggregates that were stable, except for sand particles too large to get through the screen.
17. Both sets of cans are placed in a convection oven at 110 °C until the water has evaporated.
18. The weight of the materials in each can is then determined by weighing the can, plus contents, and subtracting the weight of the can.
The fraction stable is equal to the weight of soil obtained in the "ultra sonic probe" cans divided by the sum of the weights obtained in the "ultra sonic probe" cans and distilled water cans.

Nothing in this publication may be reproduced and/or made public by means of print, photocopy, microfilm or any other means without previous written permission from Eijkelkamp Agrisearch Equipment.

Technical data can be amended without prior notification.

Eijkelkamp Agrisearch Equipment is not responsible for (personal damage due to (improper) use of the product.

Eijkelkamp Agrisearch Equipment is interested in your reactions and remarks about its products and operating instructions.

Product Evaluation Form

Thank you for using the Product Evaluation Form. The survey should take less than five minutes of your time to complete. It is also possible to fill in the form on-line. Please visit www.eijkelkamp.com.

Please rate your satisfaction level with each of the following statements.

- 1 = very satisfied 4 = somewhat dissatisfied
 2 = somewhat satisfied 5 = very dissatisfied
 3 = neutral Leave blank if not applicable

Name	<input type="text"/>	Art. no.:	<input type="text"/>				
Address	<input type="text"/>		Product	<input type="text"/>			
City	<input type="text"/>	State	<input type="text"/>	Zip Code	<input type="text"/>	Telephone	<input type="text"/>
Country	<input type="text"/>		E-mail	<input type="text"/>			

Product

	1	2	3	4	5
1. How satisfied are you with delivery of the products (complete)?	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
2. How satisfied are you with the instructions before use?	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
3. Rate your satisfaction with the product's operating instructions What is missing in the operating instructions, how can we improve it?	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
<input type="text"/>					
4. How satisfied are you with the solutions offered by the product?	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
5. How satisfied are you with time and cost savings achieved?	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
6. How satisfying is the quality of the product?	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
7. Rate your overall satisfaction with the product.	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
8. Please describe where and in what circumstances the equipment is used	<input type="text"/>				

Technical Support

9. How satisfied are you with the technical support in general?	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
10. How satisfied are you with the technical support by Eijkelkamp training & Consultancy?	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
11. Our comments:	<input type="text"/>				

12. How can Eijkelkamp improve your customer experience?